

*microlife*<sup>®</sup>

# WatchBP<sup>®</sup> Office

Professional  
Automated Office  
Blood Pressure  
Monitor



BP 3SK1-3B

## Instruction Manual

# Preface

Microlife WatchBP Office (BP3SK1 -3B) is an Automated Office Blood Pressure (AOBP) Monitor.

The device is a non-invasive digital blood pressure device using oscillometric technique and an upper-arm blood pressure cuff to measure systolic and diastolic blood pressures, pulse rate, mean arterial pressure (MAP) and pulse pressure (PP) for use in pediatric and adult populations with arm cuff circumference sizes ranging from 14 -52 cm.

The device can be connected to a computer (PC) running the WatchBP Analyzer software. The measured patient data can be transferred from the blood pressure monitor to the PC by means of a USB cable connection or Bluetooth connection. The Bluetooth 4.2 connectivity allows data transferring from the device to PC, smartphones or tablet.

The device detects the appearance of atrial fibrillation during measurement and gives a warning signal together with the measured blood pressure value if atrial fibrillation is detected (optional).

The device provides aortic blood pressure parameters, includes central systolic blood pressure (cSBP), central pulse pressure (cPP) and central diastolic pressure (cDBP), non-invasively through the use of a brachial cuff (optional).

## **WatchBP product support:**

<https://www.microlife.com/professional-products>

## **WatchBP Software support:**

<https://www.microlife.com/support/software-professional-products>

## **Developers support:**

<https://www.microlife.com/developers1>

# Table of Contents

## Product description

· Contents .....	4
· Device Version .....	4
· Upgrading the version of the device .....	4
· Product Overview .....	5
· Display .....	5

## Initial set up

· Attaching the power plug to the power adapter .....	6
· Power ON/OFF .....	6
· Set the date, time and the safeguard pressure .....	6

## Before using the device

· Selecting the correct cuff .....	7
· Fitting the cuff properly .....	7

## Taking measurements in MANUAL and AUTO Mode

· Turn on the power .....	8
· Connect the cuff to the device .....	8
· Select an operation mode .....	8
· Settings of AUTO Mode .....	8-9
· Taking measurement in AUTO Mode .....	10
· Viewing stored values .....	10
· MANUAL Mode Settings .....	10
· Taking measurement in MANUAL Mode .....	11

## Special Functions

· Screening for atrial fibrillation during blood pressure measurement .....	12
· About Atrial Fibrillation .....	12
· Central blood pressure parameters .....	12
· How is central blood pressure measured? .....	12
· Accuracy of the central blood pressure parameters .....	13
· MAP (Mean Arterial Pressure) .....	13

## Using WatchBP Analyzer

· Installing the Software Program .....	14
· Connecting the Device to a Computer .....	14
· Start the Software Program .....	14
· Transferring and deleting measurement data .....	14
· Bluetooth connectivity .....	15

## Rechargeable battery and power adapter

· Rechargeable Battery .....	15
· Using a power adapter .....	16

## Safety, care, accuracy test and disposal

· Device care .....	16-17
· Cleaning the cuff .....	17
· Accuracy test .....	17
· Disposal .....	17

## Error messages and Troubleshooting

## Technical specifications

# Product description

## The WatchBP Office consists of two major parts

- The device, cuffs and accessories.
- The WatchBP Analyzer Software.

## With the WatchBP Analyzer Software

- 1) The device can be programmed for the blood pressure measurement procedure.
- 2) Measured blood pressure values can be downloaded to the PC.
- 3) A PDF report and Microsoft Excel spreadsheet for data analysis can be generated.

\* Download the latest WatchBP Analyzer Software from the Microlife website.

<https://www.microlife.com/support/softwareprofessional-products>

## Contents

1. WatchBP Office AOBP Monitor  
(dependent on purchase version\*)
2. WatchBP Office Cuff – Size M (22- 32cm)
3. WatchBP Office Cuff – Size L (32- 42cm)
4. Data Cable
5. Mains adapter
6. Instruction manual
7. Quick start guide



## Device Version


\* The device can be upgraded with special features. There are three different versions of the device:

- **Standard version:** standard AOPM
- **AFIB version:** standard AOPM with Microlife Atrial Fibrillation Detector
- **CBP version:** standard AOPM with Microlife Atrial Fibrillation Detector and Central Blood Pressure measurement


## Upgrading the device

The Atrial Fibrillation Detector and Central Blood Pressure measurement of the device can be activated through the WatchBP Analyzer. An activation key is needed for activation, the activation key is specific for the device as it matches the ID. Please contact Microlife or the local distributor for additional information.

## Product Overview

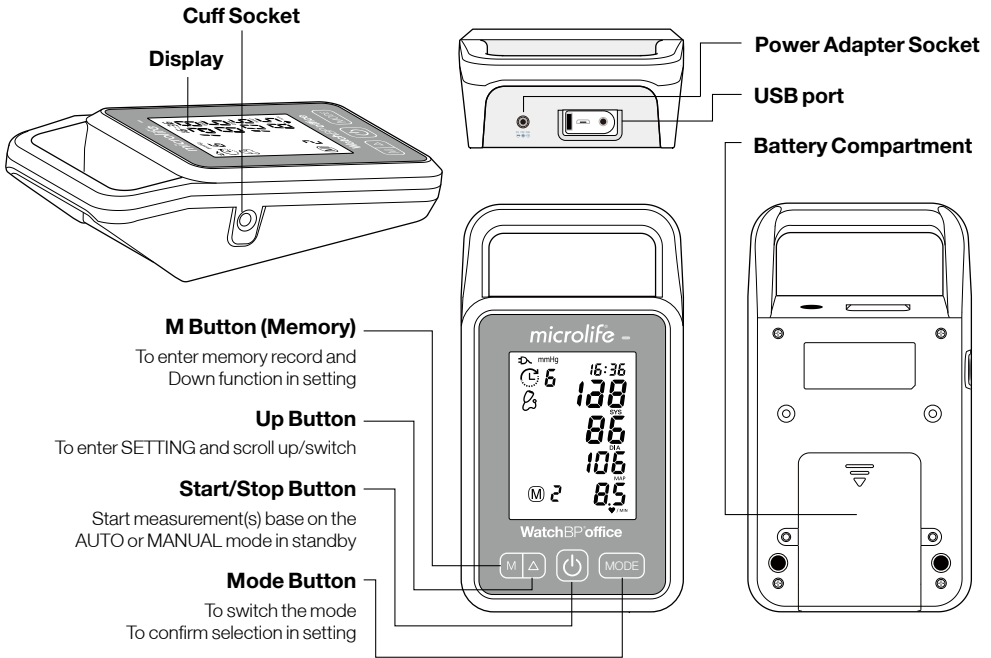

## Display

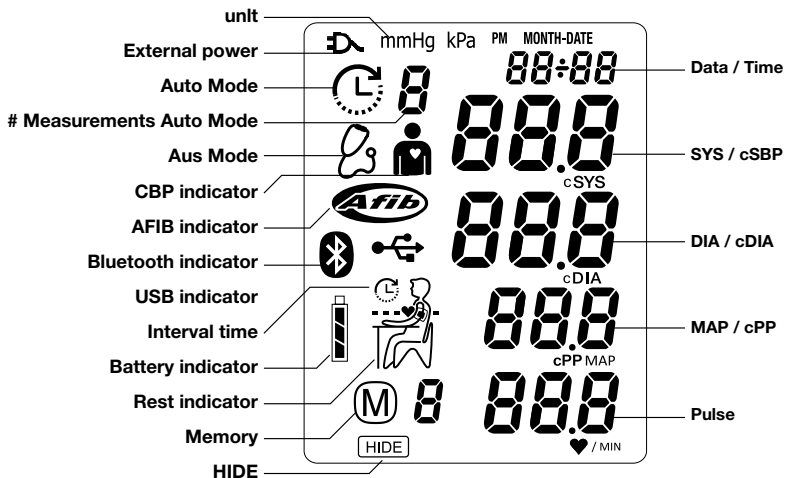


# Initial set up

## Attaching the power plug to the power adapter


Select a proper power plug and attach to the power adapter as shown below.


## Charge the battery completely

When using the device for the first time, charge the battery until the recharge indicator on the device turns green.

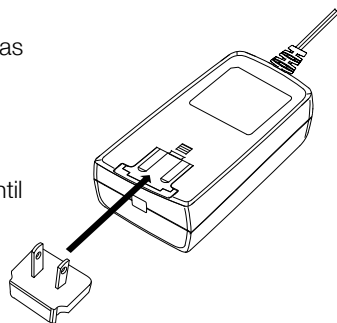








## Power ON/OFF



Press  button to switch on the device.


Press and hold  button for 3 seconds to switch off the device and turn off the LCD screen. The device displays 'oFF' before turning off.




## Set the date, time and the safeguard pressure

**Set the year** - Press and hold the  button for 3 seconds to enter setting mode. The year number flashes in the display. Use the  or  button to select the year. Use the  button to confirm your selection and move on to month setting.

**Set the month** - Use the  or  button to select the month. Use the  button to confirm your selection and move on to day setting.

**Set the day** - Press the  or  button to select the day. Use the  button to confirm your selection and move on to day setting.

**Set the time** - Once you have set the hour and minutes and pressed the  button, the date and time are set, and the current time is displayed.

**Set the safeguard pressure** - Use the  or  button to select the highest inflation pressure or AUTO mode. Use the  button to confirm and finish the settings. Once you have finished the setting mode the current time is displayed.

\* The "highest inflation pressure" can be programmed to the device. The suggested Inflation Pressure is 30 to 40 mmHg above the expected systolic value of the patient. You can select 160, 180, 200, 220 or, 240mmHg or use the default (device Displays "- - -") then the device will automatically inflate the cuff to the optimal cuff pressure. If the selected Highest Inflation Pressure selected is too low to measure a patient's blood pressure it may result in re-pumping or an error ("Err ") will be shown.

\* The date and time on the device automatically synchronizes with the date and time on the computer when connected with the WatchBP Analyzer.

# Before using the device

## Selecting the correct cuff


A variety of different cuff sizes are available. M and L size cuffs are provided with the device. Use the cuff marker to select the cuff size that best matches the circumference of the patient's upper arm.

Cuff Size	Circumference (cm)	Circumference (inch)
<b>S</b>	14-22	5.5-8.7
<b>M</b>	22-32	8.7-12.6
<b>L</b>	32-42	12.6-16.5
<b>L-XL</b>	35-52	12.5-20.5

- \* Each cuff is provided with 130 cm air tube.
- \* Use only cuffs provided by Microlife!
- \* Contact Microlife or its authorized distributor to purchase cuffs.
- \* M and L size cuffs are included as standard accessories.

## Fitting the cuff properly

- 1 Place the cuff over the upper arm so that the air tube and artery mark arrow point towards the lower arm. The artery mark on the cuff must be placed over the brachial artery.
- 2 Lay the cuff on the arm. Make sure that the lower edge of the cuff lies approximately 2 to 3 cm ( $\frac{3}{4}$  to 1 inch) above the elbow.
- 3 Wrap and tighten the cuff around the arm.
- 4 Leave free space with the size of 2 fingers between the arm of the patient and the cuff. Excessive tightness may cause venous congestion and discoloration of the limb. If the cuff is wrapped too loosely, it cannot be inflated properly, and the measured values may be inaccurate. Remove all clothing covering or constricting the measurement arm. Clothing may interfere with measurement accuracy.
- 5 Cuffs that do not fit properly may lead to inaccurate readings. Use a different size cuff if the range index at the end of the cuff does not fall into the range specified by the range stripes.

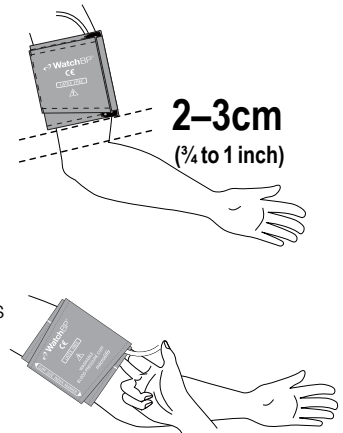

# Taking measurements in MANUAL and AUTO Mode

## Turn on the power

Turn on the device by pressing the  button of the device.


## Connect the cuff to the device

Connect the cuff to the device by inserting the cuff connector into the cuff connector socket.

## Select an operation mode





There are two measurement modes that can be used.

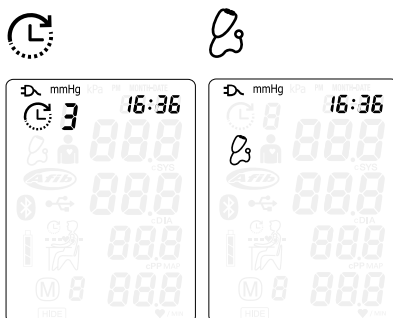
Press the  button to switch between **AUTO** or **MANUAL** Mode.






## Settings of AUTO Mode




The measurement program in AUTO Mode of the device can be set, includes **Number of Measurements**, **Resting time (Countdown time)**, **Interval time**, **AFIB detector**, **CBP measurement**, **HIDE** and **Average calculation (Discard 1st measurement)**.

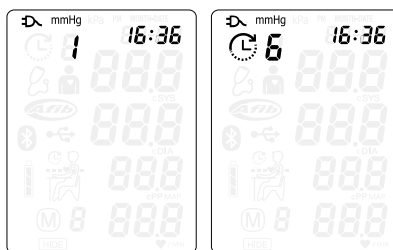**1 Set the Number of Measurements** – Press the  button when the device is in AUTO mode to first enter setting of Number of Measurements. Use the  button to scroll up and use  button to scroll down among one to six measurements. Press  button to confirm the number of measurements and enter Resting time setting.






**2 Set the Resting Time** – Press the  button to scroll up and use  button to scroll down among 15, 30, 60, 120, 180, 240, 300 seconds of resting time. Press  button to confirm and enter Interval Time setting.




**3 Set the Interval Time** – between measurements - Press the  button to scroll up and use  button to scroll down among 15, 30, 60, 120, 180, 240, 300 seconds of Interval Time. Press  button to confirm and enter Interval Time setting.






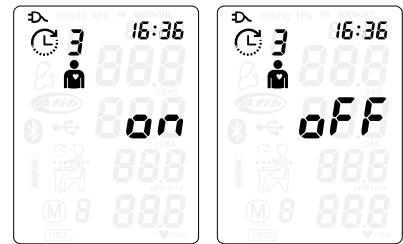




- 4 Set the Atrial fibrillation (AFIB) detector –**  
Press the  or  button to switch the **AFIB detector** ON or OFF. Press  button to confirm.

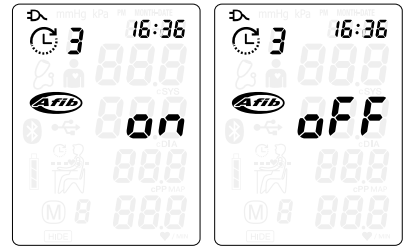
\* *Set the AFIB detector option appears only for the device version with AFIB detector. If the device has an activated AF indicator then it is switched on in Default.*






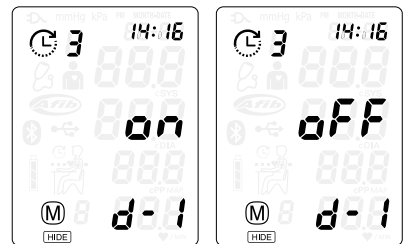
- 5 Set the Central blood pressure (CBP) measurement –** Press  or  button to switch ON or OFF **CBP measurement**. Press  button to confirm. If the device is upgraded with CBP then it is switched on in default.



- 6 Set the Hide function –** The device features a **Hide** function in order to prevent influence on blood pressure in patients due to nervousness triggered by visible blood pressure measurements. Press  or  button to switch ON or OFF the **Hide** Function.

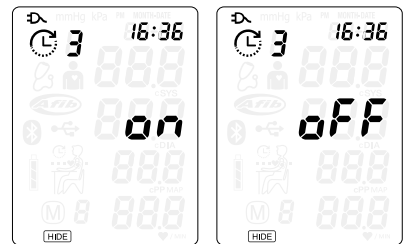


- 7 Average calculation –** The device features allow you to discard 1st measurement from averaging while the selected number of measurement is 3, 4, 5, or 6 measurements. Press  or  button to switch ON or OFF and press  button to confirm the setting of **Discarding 1<sup>st</sup> measurement (d-1)** feature and finish the setting of AUTO mode. Once you go through the settings, the device returns to standby.





\* *The last settings programmed to the device are the default of AUTO mode until you set the program again.*

## Taking measurement in AUTO Mode

Select AUTO Mode. Press the  Button to perform automatic measurements base on the settings of AUTO mode. The device shows all the settings and then starts counting down the Resting Time before the first measurement. The average measurement reading is displayed and saved after the measurements are complete.





- \* If CBP measurement is enabled, the cuff pressure is hold at around 50-150mmHg for around 10 seconds to collects sufficient pulse waves.
- \* Press Start/Stop during countdown skip the counting down.
- \* Pressing Start/Stop to deflation terminate the measurement while cuff is inflating or deflating. Display the results (average) if available.

## Viewing stored values


The device stores blood pressure values of the last measurement procedure in AUTO Mode. Press the  Button to reveal the average of the measurements of AUTO mode. Continue pressing the  Button to review individual measurements.



## MANUAL Mode Settings


The measurement program in MANUAL Mode can be set to preferences. The program includes seting the **Highest Cuff Pressure** and **Hide Cuff Pressure** during deflation.

**Set Highest Inflation Pressure** – press  button when the device is in MANUAL mode to enter setting of Highest Cuff Pressure. Use  button or  button to scroll among 160, 180, 200, 220 240 mmHg and auto '---'. Use the  button to confirm and move to **HIDE Pressure** setting.

- \* When auto '---' is selected, the device automatically inflates the cuff to a proper cuff pressure;
- \* The Highest Inflation Pressure is considered as a safeguard pressure. The device automatically inflates the cuff to the optimal cuff pressure but not higher than the selected Highest Cuff Pressure.

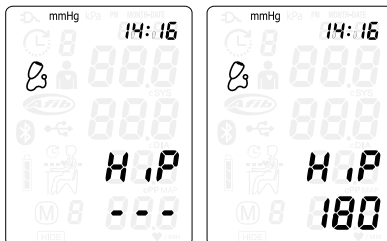

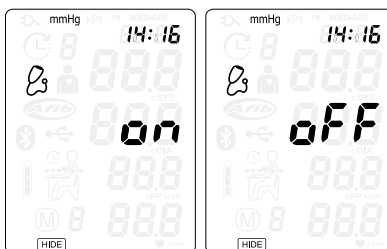


**Hide Cuff Pressure during deflation** – This option helps you to determinetake Korotkoff K1 and K5 sound readings without digit preference. To use the HIDE function in MANUAL mode, push  button to select the setting of HIDE function and confirm the selection by  button and finish the setting of MANUAL mode.




## Taking measurement in MANUAL Mode


Select the MANUAL Mode if auscultatory blood pressure measurement is preferred above oscillometric blood pressure measurement. In MANUAL Mode, the device serves as a pressure gauge. No oscillometric measurements will be taken. Systolic and diastolic Korotkoff sounds must be determined by a stethoscope placed over the brachial artery.

**Start inflation** – Press the  button to start cuff inflation. When the maximum inflation pressure is reached, the device will automatically begin a linear deflation at a rate of 3 mmHg/sec as is recommended by the guidelines.

**Assess the Korotkoff K1 and K5 sound** – when pushing the  button during cuff deflation the cuff pressure at the time of pushing is temporarily stored so that the systolic (K1) and diastolic (K5) pressures can be seen afterwards. The device can store up to 4 pressures. Push the  button at any time to start fast deflation and finish the measurement of MANUAL mode and show the pressure you have marked. Alternatively, the device quickly deflates and shows the pressures after having pushed the button 4 times, or the cuff pressure has reached 20mmHg during the deflation cycle.

After the measurement in MANUAL mode, the device displays all marked cuff pressures for one minute.

**Re-inflate** – Push and Hold the Up  button during deflation to re-inflate for as long as the button is held up to a max of 299mmHg. Release the button to continue deflation. Exceeding 299 mmHg will result in an immediate release of cuff pressure and a 'HI' Error message.

**Deflate faster** – Push and hold the  button when deflation will releases the pressure in the cuff faster, at around 8 -12 mmHg/second.

\* The recommended deflation rate for auscultation is 2-3 mmHg per seconds. Do not assess K1 or K5 sound while holding the M button.

\* If Hide of the MANUAL mode is selected, the cuff pressure during deflating the cuff will not be displayed. The display shows '---' during deflating the cuff

# Special Functions

## Screening for atrial fibrillation during blood pressure measurement

The device is designed to screen for atrial fibrillation during blood pressure measurements (optional) with high accuracy: a sensitivity of 98% and a specificity value of 92%\*. If atrial fibrillation is detected this will be shown in the report.

 Verberk et al. Screening for atrial fibrillation with automated blood pressure measurement: Research evidence and practice recommendations. *Int J Cardiol* 2016: 465–473.

## About Atrial Fibrillation

Atrial fibrillation is a common heart rhythm problem and a common cause of major strokes. It affects 8% of those 65 years and older and about 20% of all strokes are caused by atrial fibrillation. Atrial fibrillation is a rhythm problem that can last from a few minutes, to days or weeks and even years. Atrial fibrillation can lead to the formation of blood clots in the heart. These clots can break off and flow to the brain causing stroke. One sign of atrial fibrillation is palpitations. However, many people have no symptoms and therefore may remain undetected whereas diagnosing atrial fibrillation early followed by adequate treatment can largely reduce the chance of getting a stroke.

## Central blood pressure parameters

The device is designed to assess central blood pressure parameters (optional).

Central blood pressure is the pressure in the ascending aorta, the largest artery that originates from the left ventricular of the heart and from where oxygen is distributed to all parts of the body through the systemic circulation. Central Systolic Blood Pressure and Central Pulse Pressure provided by this monitor are determined directly through pulse volume plethysmography (PVP) waveform analysis. Central Diastolic Blood Pressure by this monitor is calculated by subtraction of Central Systolic Blood Pressure and Central Pulse Pressure.


## How is central blood pressure measured?


The device measures brachial systolic and diastolic blood pressure as usual. However, where the cuff normally totally deflates after the blood pressure measurement, the cuff now stops deflating at approximately 60 mmHg cuff pressure to keep a stable pressure on the brachial artery for approximately 10 seconds which is needed to acquire brachial pulse volume plethysmography (PVP) waveforms (pulse volume recording). During these 10 seconds approximately 10 PVP waveforms are recorded from which one average PVP waveform is determined and analyzed. From the average PVP waveform, some characteristic points (parameters) are identified that are directly related to arterial compliance (stiffness) and wave reflections. With these parameters and previously measured peripheral (regular) blood pressure the central systolic blood pressure value and the central pulse pressure value are then determined<sup>1</sup>.

The time that is needed to determine the central blood pressure value may vary among patients; i.e. with faster heart rate, less time is required for collecting the number of required PVP waveforms. It is very important to keep the arm still during the time the PVP waveforms are collected.

### Accuracy of the central blood pressure parameters

The accuracy of central blood pressure parameters performed with this device can only reliably be determined against intra-arterial blood pressure measurement. The device is a certified equivalence with the WatchBP Office Central that has been validated against simultaneous recorded intra-arterial blood pressure measurement in 85 subjects and showed high accuracy<sup>2</sup>.

 Sung, S.H., et al., Measurement of central systolic blood pressure by pulse volume plethysmography with a noninvasive blood pressure monitor. *Am J Hypertens*, 2012, 25: 542-8.

 Cheng, H.M., et al., Measurement accuracy of a stand-alone oscillometric central blood pressure monitor: a validation report for Microlife WatchBP Office Central. *Am J Hypertens*, 2013, 26: 42-50.

### MAP (Mean Arterial Pressure)

The device measures the true mean arterial pressure (MAP) of the patient. Each measurement includes a single MAP value. The MAP value will always be displayed together with the systolic and diastolic blood pressure value.

# Using WatchBP Analyzer

## Installing the Software Program

The latest WatchBP Analyzer Software is available from the Microlife website.

<https://www.microlife.com/support/softwareprofessional-products>

Double click the download installer and simply follow the instructions provided in the installation window on the computer screen.

## Connecting the Device to a Computer


Connect the device to the PC using the USB cable provided with the device.

## Start the Software Program

Start the software program. The date and time on the device automatically synchronizes with the date and time on the computer when successfully connected with WatchBP Analyzer PC software.

If the device and WatchBP Analyzer software is connected successfully:

- <USB> is displayed on the LCD screen of the device.
- The device ID, model, version of the Device and batteries condition etc. are displayed on the WatchBP Analyzer software.

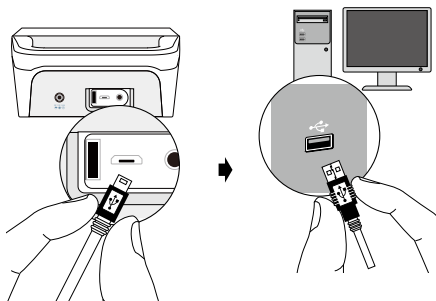



## Transferring measurement data

Connect the device to the PC. Start the WatchBP Analyzer software program.

Click <Download> button of the WatchBP Analyzer to transfer the measurement data on the device to a computer.

## Deleting measurements

The measurement data on the device will be automatically deleted after clicking <Program Device> in the WatchBP Analyzer software to program a measurement schedule for the next patient.

\* Press and hold  button of the device for 7 seconds displays CL, presses  button again to clear the memory



 See instruction manual of WatchBP Analyzer for details.

# Bluetooth connectivity

## Pairing the device

Press and hold the **MODE** button for around 7 seconds, until the Bluetooth icon flashes and starts pairing mode. The unique 6-digit device ID of the unit is displayed. Connect the device and confirm pairing. The Bluetooth icon is displayed on the LCD screen of the device to show the presence of Bluetooth connection.

 Press and hold the Start/Stop button for 5 seconds to clear the connection.

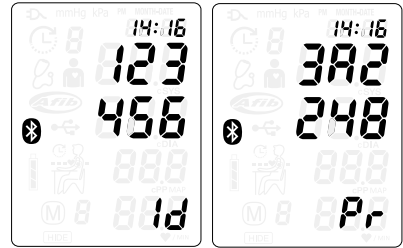

# Rechargeable battery and power adapter

## Rechargeable Battery

The device has a built-in, rechargeable Ni-MH battery pack that can perform up to 400 measurement cycles on a full charge. The battery can be recharged with the power adapter delivered with the device. The empty battery indicator is displayed when the battery is low.


- When using the device for the first time, charge the battery until the recharge indicator turns to green.
- The orange recharge indicator indicates that the recharge is in progress.
- A green recharge indicator indicates that the recharge is completed.
- A green and orange changing recharge indicator, means that there is a charging error. Make sure that of the correct Mains Adapter is used. If the condition persists, contact Microlife or the local distributor.



## Using a power adapter

Only use the Mains Adapter supplied with the device to recharge the device.

- 1) Plug the adapter cable into the power socket of the device.
- 2) Plug the adapter plug into the wall socket.  
The battery will be recharged if the device is attached to an AC power source. After the battery is fully recharged, the charging will stop. No battery power will be used if the adapter is plugged in. The battery must always remain within the device thus also when using AC power.
- 3) If the battery starts losing capacity, contact your local dealer for replacement battery. The battery can be replaced.

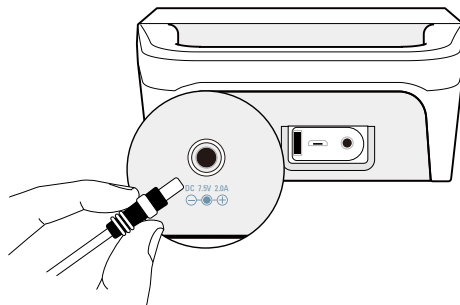

## Safety, care, accuracy test and disposal

### Safety and protection

This device may only be used for the purposes as described in these instructions. The device comprises of sensitive components and must be treated with caution. The manufacturer cannot be held liable for damage caused by incorrect application.



Follow the Instructions for Use. This document provides important product operation and safety information regarding this Blood Pressure Monitor. Please read this document thoroughly before using the device and keep for future reference.



- Only activate the pump when the cuff is connected to the device.
- Do not use the device if you think it is damaged or if anything appears unusual.
- Read the further safety instructions in the individual sections of the instruction manual.



Observe the storage and operating conditions as described in the “Technical specifications” section of this manual.



**Protect the device from water and moisture**



**Protect the device from direct sunlight**



**Protect the device from extreme heat and cold**



**Avoid proximity to electromagnetic fields, such as those produced by mobile phones**



**Never open the device**




**Protect the device from impact and drops**

### Device care

Use a soft cloth with one of the following recommended cleaning solutions to wipe the exterior of the device:


- Mild soap and water.
- Hydrogen peroxide solution (3% diluted with water).
- Sodium hypochlorite solution (1:10 dilution of household chloride bleach in water).

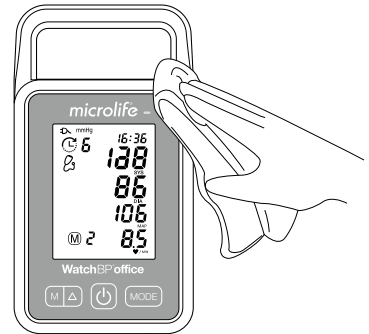

### Cleaning the cuff

Remove the bladder. Fold and place the cuff cover inside a washing bag. Wash the cuff cover with warm water (43°C; 110°F) and a mild detergent in the washing machine.

**Pasteurization:** wash the cuff cover in 75°C(167°F) hot water for 30 minutes.

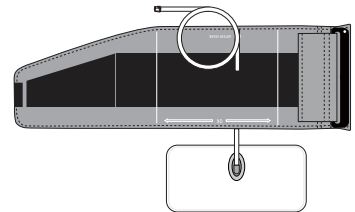

### Accuracy test

We recommend the device to be tested for accuracy every 2 years or after mechanical impact (e.g. Being dropped). Please contact Microlife to arrange an accuracy test.



**Do not iron the cuff!**




### Disposal

Batteries and electronic instruments must be disposed of in accordance with the locally applicable regulations, and not as domestic waste.

# Error messages and Troubleshooting

If an error occurs during measurement, the measurement is interrupted and an error message «Er» is displayed.




Error	Description	Potential cause and remedy
"Er 1"	Signal too weak	The pulse signals on the cuff are too weak. Reposition the cuff and repeat the measurement.
"Er 2"	Error signal	During the measurement, error signals were detected by the cuff, caused for instance by movement or muscle tension. Repeat the measurement, keeping your arm still.
"Er 3"	No pressure in the cuff	An adequate pressure cannot be generated in the cuff. A leak may have occurred. Replace the blood pressure cuff if necessary. Repeat the measurement.
"Er 5"	No valid results	The measuring signals are inaccurate, and no result can therefore be displayed. Read through the checklist for performing reliable measurements and then repeat the measurement.
"Er 11"	Signal too weak during central blood pressure measurement	The pulse signals on the cuff are too weak. Re-position the cuff and repeat the measurement.
"Er 12"	Error signal during central blood pressure measurement	During the measurement, error signals were detected by the cuff, caused, for instance, by movement or muscle tension. Repeat the measurement, when keeping the arm still.
"Er 13"	Cuff pressure errors during central blood pressure measurement	An adequate pressure cannot be generated in the cuff. A leak may have occurred. Check if the cuff is correctly connected and is not too loose. Replace the blood pressure cuff if necessary. Repeat the measurement.

<b>"Er 15"</b>	<b>Abnormal result of central blood pressure reading</b>	The measuring signals are inaccurate so that no result can be displayed. Read through the checklist for performing reliable measurements and then repeat the measurement.
<b>"Er F"</b>	<b>The device has gone into "single fault condition"</b>	Single fault condition means that the measurement is aborted to protect the patient from being harmed or the device from being damaged. Re-position the cuff and repeat the measurement. Replace the batteries if necessary. If the error persists, contact Microlife or the local distributor.
<b>"Er A"</b>	<b>Flash memory error</b>	Possible hardware fault. Try again. If the error persists, contact Microlife or the local distributor.
<b>"HI"</b>	<b>Pulse or cuff pressure too high</b>	The pressure in the cuff is too high (over 299 mmHg) OR the pulse is too high (over 239 beats per minute). Relax for 5 minutes and repeat the measurement.
<b>"LO"</b>	<b>Pulse too low</b>	The pulse is too low (less than 30 beats per minute). Repeat the measurement.

## Troubleshooting

<b>Problem</b>	<b>Possible cause</b>	<b>Solutions</b>
<b>No power (No LCD display)</b>	<b>Power supply is not properly plugged in</b>	Plug the power supply into the wall socket.
	<b>Battery is fully discharged</b>	Recharge the rechargeable battery by plugging in the power supply.
<b>Cuff does not inflate properly</b>	<b>Loose connection of the tube</b>	Make sure the tube of the cuff is securely connected to the device.
	<b>Leakage of the tube / bladder</b>	Check for cracks on the tube or the bladder. Replace the blood pressure cuff if necessary.
<b>No result displayed after measurements</b>	<b>Device is in MANUAL Mode</b>	Switch to AUTO Mode and repeat the measurements.

# Technical specifications

<b>Operation temperature/ humidity:</b>	<ul style="list-style-type: none"><li>• 10 to 40 °C (50 to 104 °F)/ 15 - 90 % relative maximum humidity</li></ul>
<b>Storage temperature/ humidity:</b>	<ul style="list-style-type: none"><li>• -20 to 55 °C (-4 to 131 °F)/ 15 - 90 % relative maximum humidity</li></ul>
<b>Weight:</b>	<ul style="list-style-type: none"><li>• 620g (including rechargeable battery pack) (to be measured by real/final sample)</li></ul>
<b>Dimensions:</b>	<ul style="list-style-type: none"><li>•  x      mm</li></ul>
<b>Measuring method:</b>	<ul style="list-style-type: none"><li>• Oscillometric, Systolic blood pressure = K1; Diastolic blood pressure = K5</li></ul>
<b>Measurement range:</b>	<ul style="list-style-type: none"><li>• 60 - 255mmHg - systolic blood pressure; 30 - 200mmHg - diastolic blood pressure; 30 - 239 beats per minute - pulse</li></ul>
<b>Cuff pressure display:</b>	<ul style="list-style-type: none"><li>• Range: 0 - 299 mmHg; Resolution: 1 mmHg; Static accuracy: pressure within ± 3 mmHg;</li></ul>
<b>Pulse accuracy:</b>	<ul style="list-style-type: none"><li>• ±5 % of the readout value</li></ul>
<b>Power source:</b>	<ul style="list-style-type: none"><li>• Rechargeable battery pack; 4.8V 2400 mAh; Mains power supply DC 7.5V, 1.5 A</li></ul>
<b>Expected service life:</b>	<ul style="list-style-type: none"><li>• 2 years</li></ul>
<b>Reference to Standards:</b>	<ul style="list-style-type: none"><li>• Device corresponds to the requirements of the standard for non-invasive blood pressure monitor. IEC 60601-1: 2005+A1:2012 IEC 60601-1-2: 2007/AC:2010 ANSI/AAMI/ISO 81060-2 ANSI/AAMI/ISO/IEC 80601-2-30</li></ul>

<b>Electromagnetic Compatibility:</b>	<ul style="list-style-type: none"><li>• Device fulfills the stipulations of the standard IEC 60601-1-2.</li></ul>
---------------------------------------	---

CE0044

The stipulations of the EU Directive 93/42/EEC for Medical Devices Class all have been fulfilled.



Type BF applied part

Microlife reserves the right to alter technical specifications without prior written notice.

This device is covered by a two-year guarantee from the date of purchase.

This guarantee is valid only on presentation of the guarantee card completed by the owner confirming date of purchase or purchase receipt. Batteries and wearing parts are not covered by this guarantee.

**Name:** \_\_\_\_\_

**Address:** \_\_\_\_\_

**Date:** \_\_\_\_\_

**Telephone:** \_\_\_\_\_

**Email:** \_\_\_\_\_

Product: **WatchBP Office**

Product number: **BP3SK1-3B**

Date:







## **Europe / Middle-East / Africa**

 Microlife AG

Espenstrasse 139

9443 Widnau, Switzerland

Tel. +41 71 727 7000

Fax. +41 71 727 7011

Email: [watchbp@microlife.ch](mailto:watchbp@microlife.ch)

[www.watchbp.com](http://www.watchbp.com)

***microlife®***

## **Asia**

Microlife Corporation

9F., No.431, Ruiguang Rd., Neihu Dist.,

Taipei City 114, Taiwan (R.O.C.)

Tel. +886 2 8797 1288

Fax +886 2 8797 1283

Email: [watchbp@microlife.com.tw](mailto:watchbp@microlife.com.tw)

[www.watchbp.com](http://www.watchbp.com)

## **North / Central / South America**

Microlife USA, Inc.

1617 Gulf to Bay Blvd

2nd Floor, Suite A

Clearwater, FL 33755, USA

Tel. +1 727 442 5353

Fax +1 727 442 5377

Email: [msa@microlifeusa.com](mailto:msa@microlifeusa.com)

[www.watchbp.com](http://www.watchbp.com)

**CE0044**